



Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

Product	REJUV 25mg (BPC-157/TB-500/KPV/GHK-Cu)
Net Peptide Content	GHK-Cu: 10.327 mg KPV: 4.640 mg BPC-157: 5.563 mg Thymosin Beta4: 3.952 mg
Identity	GHK-Cu/KPV/BPC-157/ Thymosin Beta4

Certificate of Analysis



Assession Number	2506060047
Client	Peptide Pro
Search Code	pept2506060047

Received Date:	6/6/2025
Reported Date:	6/10/2025

Lot	REJUV-050125
Purity	GHK-Cu: 42.62% KPV: 19.15% BPC-157: 22.96% Thymosin Beta4: 15.07%
Appearance	Blue Lyophilized Powder

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification	Result
GHK-Cu/KPV/BPC-157/Thymosin Beta4	99.80%

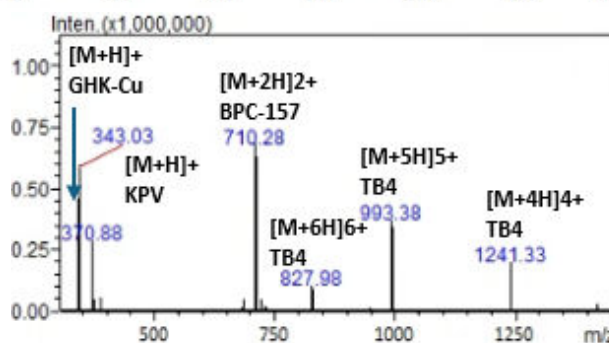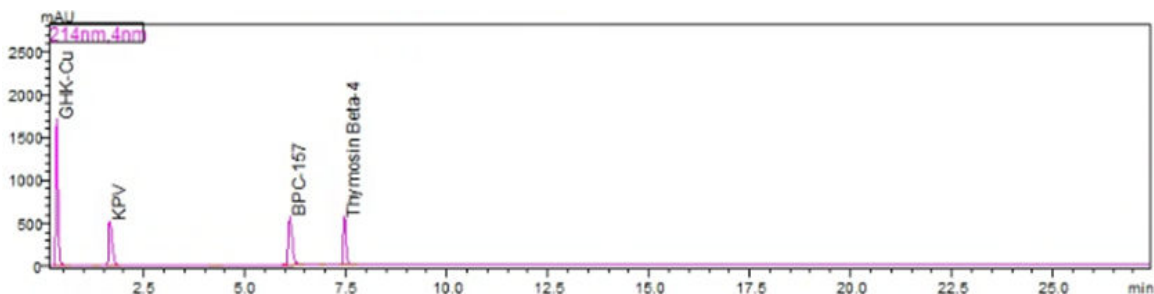

Stephen Schmidt

Stephen Schmidt
Principle Chemist

COA: 2506060047

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: FreedomDiagnosticsTesting.com

Contact at: Admin@FreedomDiagnostics.net



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Product	REJUV 25mg (BPC-157/TB-500/KPV/GH K-Cu)
----------------	---

Certificate of Analysis

Assession Number	2506060048
Client	Peptide Pro
Search Code	pept2506060048

Received Date:	6/6/2025
Reported Date:	6/9/2025

Lot	REJUV-050125
------------	--------------

All analyses are conducted for research purposes and performed in duplicate in accordance with USP <85> guidelines

Endotoxin Threshold		Result
Replicate 1	≤ 0.05 EU/mL	PASS
Replicate 2	≤ 0.05 EU/mL	PASS



Stephen Schmidt

Stephen Schmidt

Principle Chemist

COA: 2506060048

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: Admin@FreedomDiagnostics.net